

Application Note No. 078

The Thermal Desorption / Pyrolysis of Glass Fibre Air Filters

Diane Nicholas

- *Direct desorption of analytes from sample matrix to column*
- *Multi-step thermal desorption followed by pyrolysis of same sample in injector*
- *Can be automated using the CombiPAL and LINEX*

Keywords:

Pyrolysis, thermal desorption, in-injector pyrolysis, multi mode inlet pyrolysis

Instrumentation

- ATAS GL Optic 2-200 programmable injector
- Agilent 5890 gas chromatograph with 5971 mass selective detector
- SGE CO₂ cryotrap

Sample analysed

Borosilicate glass air filters impregnated with 5 % phenolic and epoxy resins and some fluorocarbons.

Principles

- Place 2-4 mg of filter paper in a fritted liner, place in injector and start run
- Liner is firstly swept and the cryotrap turned-on
- The analytes are thermally desorbed under static flow conditions
- The analytes are swept onto the column with a small split flow and trapped
- The cryotrap is turned off and the separation and analysis is performed
- At the end of the run the injector and oven are cooled and the sample is pyrolysed, following the same principles

Chromatograms

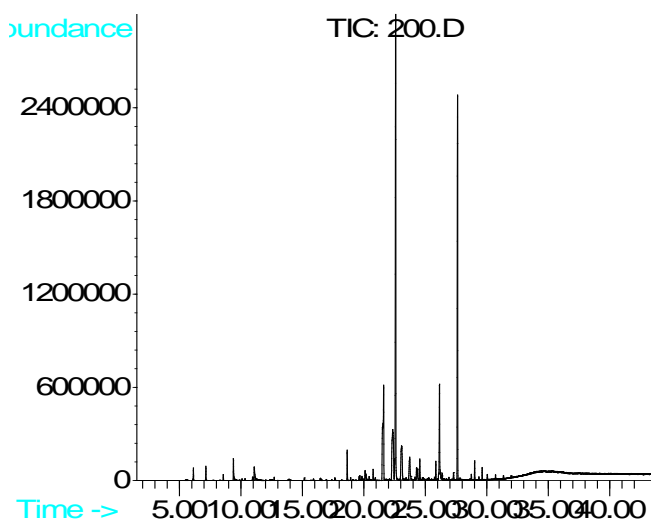


Figure 1: Filter A: Thermal desorption at 200 °C

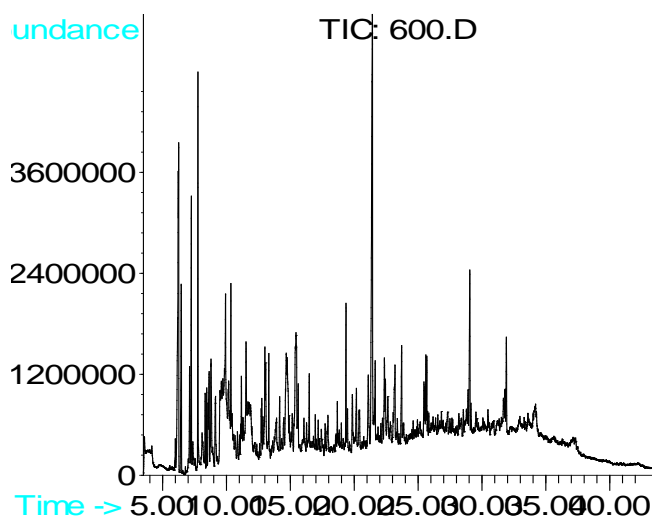


Figure 2: Filter A: Pyrolysis at 600 °C

We would like to thank Dr Anthony Lawson from Hollingworth & Vose Co Ltd. for his kind permission to publish this data

GL Sciences B.V.

Tel. +31 (0)40 254 95 31 E-mail: info@glsciences.eu
Internet: www.glsciences.eu

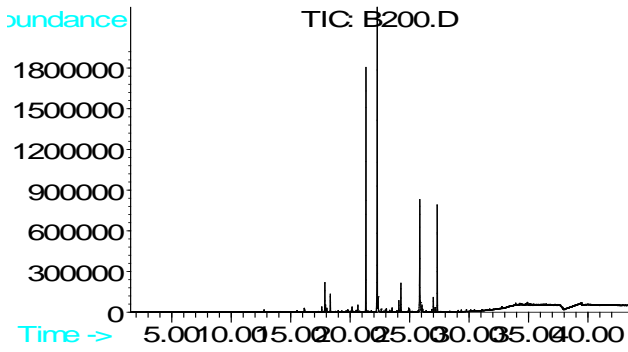


Figure 3: Filter B: Thermal desorption at 200 °C

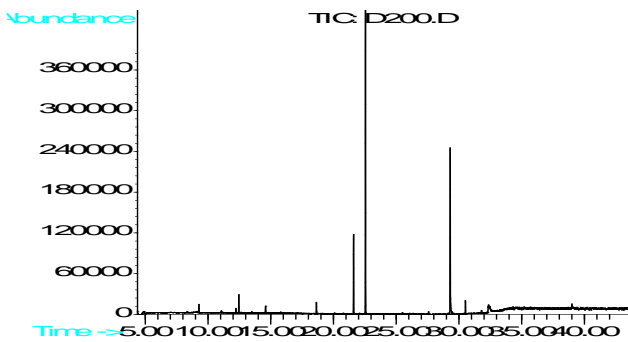


Figure 5: Filter D: Thermal desorption at 200 °C

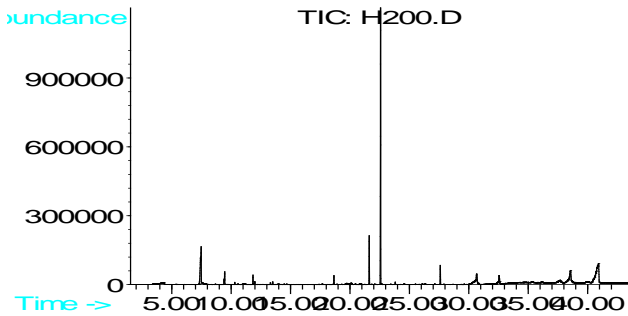


Figure 7: Filter H: Thermal desorption at 200 °C

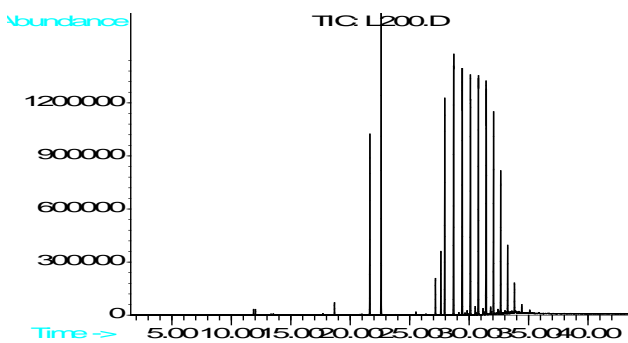


Figure 9: Filter L: Thermal desorption at 200 °C

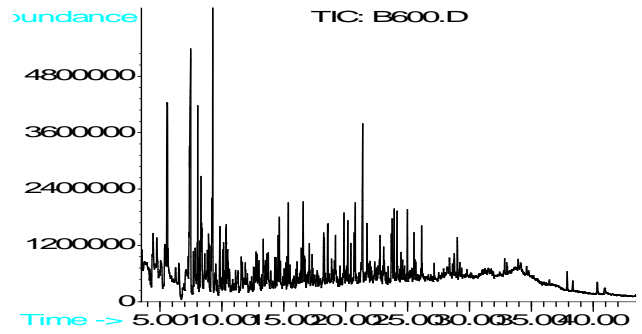


Figure 4: Filter B: Pyrolysis at 600 °C

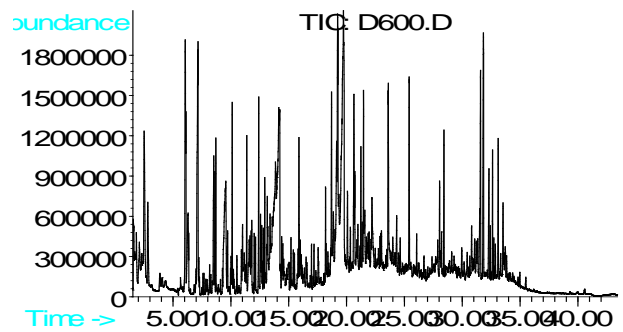


Figure 6: Filter D: Pyrolysis at 600 °C

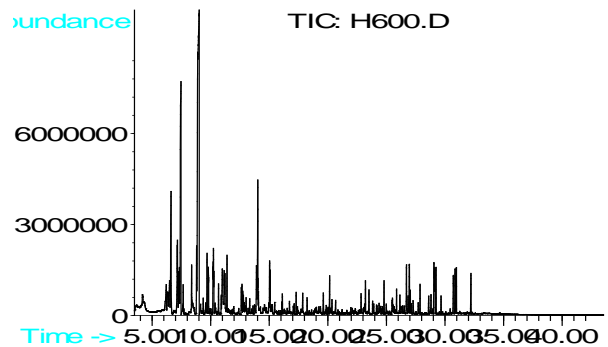


Figure 8: Filter H: Pyrolysis at 600 °C

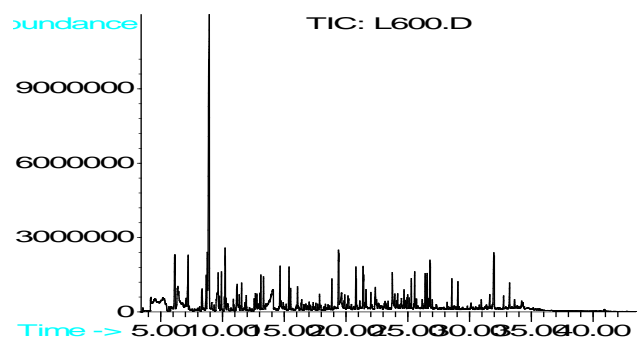


Figure 10: Filter L: Pyrolysis at 600 °C

Appendix

Optic Parameters:

Liner:	ATASGL Fritted
Mode:	Expert
Gas Flows:	Vent: 75 ml/min
	Split: 10 ml/min
Initial temperature:	35 °C
Isothermal time:	1 min
Ramp rate:	16 °C/s
Final temperature:	200 °C (thermal desorption)
Final temperature:	600 °C (pyrolysis)
End time:	43.5 mins
Sweep pressure:	8 psi
Sweep time:	0.5 mins
Split open time:	0.5 mins
Desorption pressure:	0 psi
Desorption time:	2.5 mins
Transfer pressure:	7.1 psi
Transfer time:	2 mins
Initial pressure:	7.1 psi
Final pressure:	24.8 psi

Cryotrap Parameters:

Cryo on:	0.25 mins
Cryo off:	4 mins

GC Parameters:

Column:	HP5-MS 30m x 0.25mm i.d. x 0.25um film
Initial temperature:	45 °C
Initial time:	5 mins
Ramp rate:	10 °C/min
Final temperature:	330 °C
Final time:	10 mins

MS Parameters:

Acquisition mode:	Scan
Low mass:	50 m/z
High mass:	300 m/z
Sampling number:	2
Threshold:	500
Transfer line:	330 °C
Solvent delay:	2 mins